



**Anatomic Radial
Head System**

Anatomic Radial Head System

Acumed is an industry leader in innovative solutions for extremities and trauma.

We are dedicated to pioneering solutions that benefit the patient and drive the industry forward.



Acumed's Anatomic Radial Head Prosthesis is designed to provide a precise anatomical implant to replace the patient's native radial head. Many innovative design features are incorporated into the implant heads and stems, as well as the instrumentation to improve the surgical technique.

The Anatomic Radial Head System is a comprehensive solution for radial head fractures. The Acutrak 2[®] Mini and Micro Instruments are included in the base of the tray, as well as the Locking Radial Head Plate System.

With the Anatomic Radial Head System, the surgeon is equipped with the tools needed to properly restore the patient's anatomy in a radial head replacement surgery.



Designed in conjunction with Shawn W. O'Driscoll, Ph.D., M.D., Acumed's Anatomic Radial Head System provides a comprehensive solution for radial head replacement.

Radial head fracture is the most common bony injury to the adult elbow.⁴ Current and past designs of radial head prostheses have had a round radial head component. The radial head is clearly not round but has a more ellipsoidal shape.⁴ Acumed's Anatomic Radial Head Prosthesis is a unique implant that closely replicates the natural anatomy of the patient's radial head.

Surgeons have emphasized the importance of restoring the biomechanical properties of the native radial head when radial head replacement is indicated.⁹ Acumed's system restores the proper radial head geometry along with the proper height and placement in the radial canal. Dr. O'Driscoll hypothesized that if he could not possibly fix the radial head then it should be replaced with a prosthesis that best replicates the anatomy of the patient. This could improve "tracking" with the capitellum, reduction in implant loosening and thus result in an improved patient outcome.

There are three potential areas of clinical importance of an anatomic (noncircular) radial head prosthesis: kinematics and stability, radiocapitellar contact forces, and stresses on the prosthesis-bone interface.⁹ There is a growing concern among surgeons that suggests a need for an anatomic prosthesis. Because a round radial head prosthesis is non-anatomic, and therefore does not track properly against the capitellum, the altered kinematics could affect joint function and elbow stability. More importantly, eccentric loading potentially can alter radiocapitellar contact stresses leading to either insufficient or excessive load bearing. Finally, eccentric loading will increase stress on the prosthesis-bone interface, increasing the risk for loosening.³

By providing the patient with an anatomical prosthesis, wear on the capitellum is theoretically reduced due to the improved biomechanics and balancing within the elbow. The result is less pain for the patient and a reduced chance of long-term prosthesis loosening.

For radial head fractures that indicate joint replacement, this system provides the surgeon with advanced instrumentation that is designed to properly determine the overall length of the radius. A straightforward, reproducible surgical technique aids with accurate implant insertion and placement. Innovative implant design and insertion procedure makes Acumed's Anatomic Radial Head System the next generation in radial head replacement.

Anatomic Radial Head Features


Anatomic Radial Heads and Stems replicate the patient's natural radial head geometry. The offset anatomic dish on the proximal end of the radial head implant provides improved articulation with the capitellum. The neck angle is 4 degrees, maintaining the proper angled relationship between the radial neck and the plane of the head.



Straightforward Instrumentation includes a unique collar height gauge for an improved method of determining overall length of the radius. Color-coded broaches, trial heads and stems provide quick distinction between system components and sizes. Collar reamers are included in the system to create a perpendicular neck surface for the stem collar.



200 Head and Stem Combinations provide the surgeon with an implant that matches the patient's natural anatomic radial head and neck shape. 20 standard stem options in five diameters, each have four collar height options to provide proper restoration of the overall length of the radius. The anatomical heads are provided in five diameters, left and right, to accommodate various patient sizes.

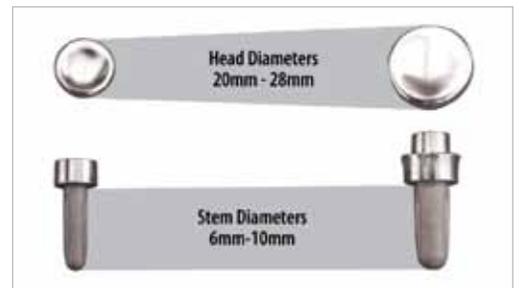

Medial Defined Ulna Articular Zone is angled and smooth to improve contact with the radial notch.

Multiple Collar Heights to restore radial length.



10mm



25mm

Highly-Polished Cobalt Chrome Head to maximize articulation.





Contoured Lateral Surface improves interface with the annular ligament.

Fluted Stem for rotational stability.

25mm Stem Length is long enough to provide stability against bending movements but short enough not to reach the bend in the proximal canal.

Grit Blasted Stem Surface promotes bony ongrowth.

Head Design Rationale

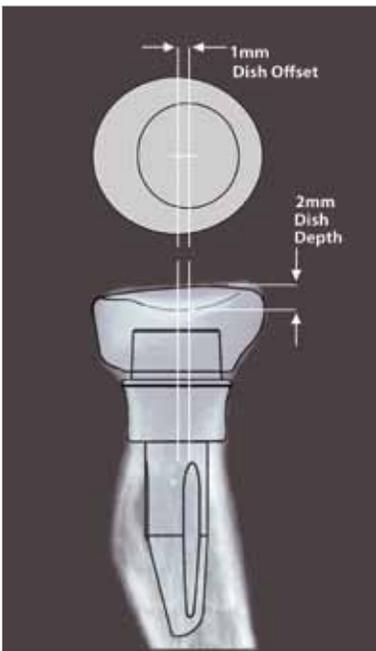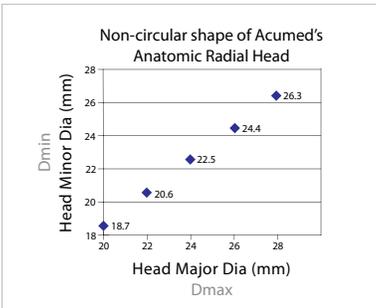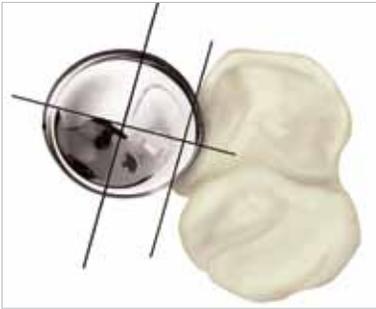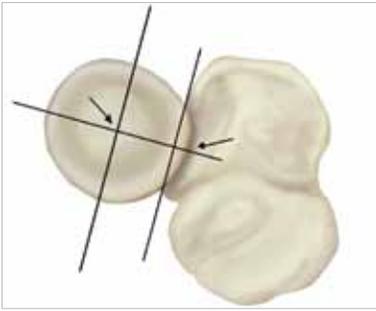

While more simple fractures of the radial head are managed with conservative treatment or internal fixation, radial head replacement may be necessary for more complex fractures. The Acumed Anatomic Radial Head Prosthesis was designed to treat those fractures not amenable to internal fixation. During the design of the prosthesis, Dr. Shawn O'Driscoll hypothesized the following:


- 1) If perfect anatomy could be restored with rigid internal fixation, that would be the best.
- 2) If we knew which aspects of the radial head shape and orientation were important, and if we could reproducibly position the prosthesis and assure fixation in the shaft, we might achieve #1.
- 3) Chances are that PERFECT replication of anatomy is not critical, but some elements are necessary.
- 4) With more research, we will determine which factors are critical.
- 5) Current trend of bipolar design is only necessary if we cannot achieve #4.

With 200 standard implant options and precise instrumentation, the Anatomic Radial Head System from Acumed is the first system that has design features that most closely replicate the patient's anatomy.





Acumed's Anatomic Radial Head Prosthesis features an elliptical-shaped head. Results of several studies, including an in-house study, have shown a strong correlation between the radial head's major diameter (D_{max}) and minor diameter (D_{min}) measured in cadaveric radial heads.¹¹ As shown in the figure to the right, the orientation of the major diameter axis is perpendicular to the radial notch when the forearm is neutral position.^{1-5,10}

A laser mark on the prosthesis head and stem components allows for proper alignment during assembly and insertion. The laser mark is located 30 degrees from the major axis. When inserting the prosthesis, the laser mark is then oriented laterally with the forearm in neutral position.⁴ Lister's tubercle may also be used as a landmark for laser mark orientation.

The dish is offset 1mm laterally from the center of the radial head to properly accommodate the patient's anatomy. The dish depth is 2mm, and is consistent amongst all implant diameters. A head height of 10mm was found to most closely replicate cadaveric radii. This was confirmed on the same 24 cadaver radii and in the referenced literature.^{3,5,6}

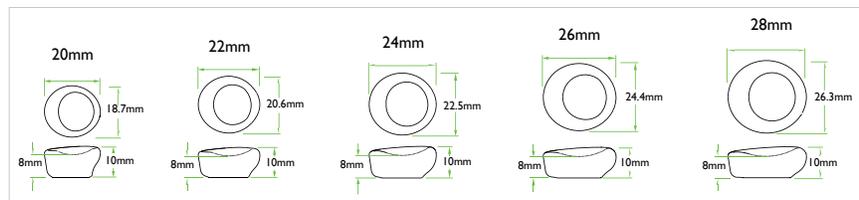

The Anatomic Radial Head was designed with 4 degrees of tilt in two planes: anterior/posterior and medial/lateral. The head tilt relative to canal axis was measured in 24 cadaver radii by drilling an oversized hole in the radial head and sequentially broaching until canal cortex met. The oversized hole allowed the broach to self align with the neck canal axis. A flat plate with a central hole was inserted over the broach and placed flat on top of the head. The angle of the head relative to the neck canal axis in the M/L plane (θ_1) and A/P plane (θ_2) was recorded along the major and minor axes. As a result of these measurements, a 4 degree M/L and A/P tilt was selected, thus creating a need for both left and right heads.¹¹

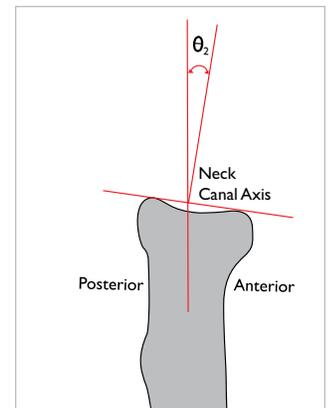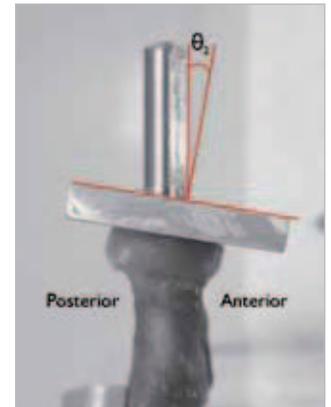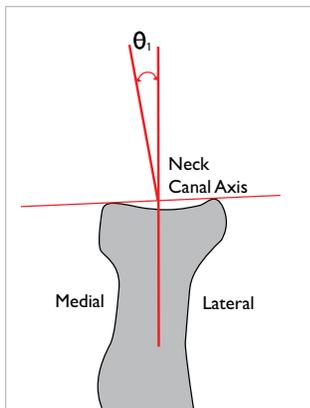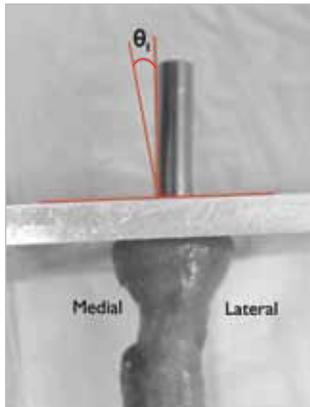


Stem Design Rationale

With the Anatomic Radial Head Prosthesis, height is restored by collar height, not the head height. Studies show that the length of the radial neck affects the valgus-varus position of the ulna throughout the flexion arc in each of the forearm rotations. Restoration of proper axial length of the radius is critical to avoid a number of complications such as residual instability.^{7,8} The shape of the collar helps to restore the natural shape of the bone. The highly polished collar minimizes soft tissue irritation.

The stem is made from titanium alloy and is designed to press fit into the neck canal. The distal portion of the stem is angled, allowing for easier insertion. The angle also allows the stem length to be longer within the radial canal for stability and to resist loosening.

The stem is grit blasted for bony ongrowth. Flutes are also added to the stem to allow for rotational stability upon bony ongrowth. A Morse taper ensures a secure fit between the collar and the head, and 20 standard and five optional stem options give the surgeon a wide range of choices when choosing proper stem diameter and collar height. A threaded hole is located in the top of the stem to allow for implant removal when used in conjunction with the removal tool, included in the system.

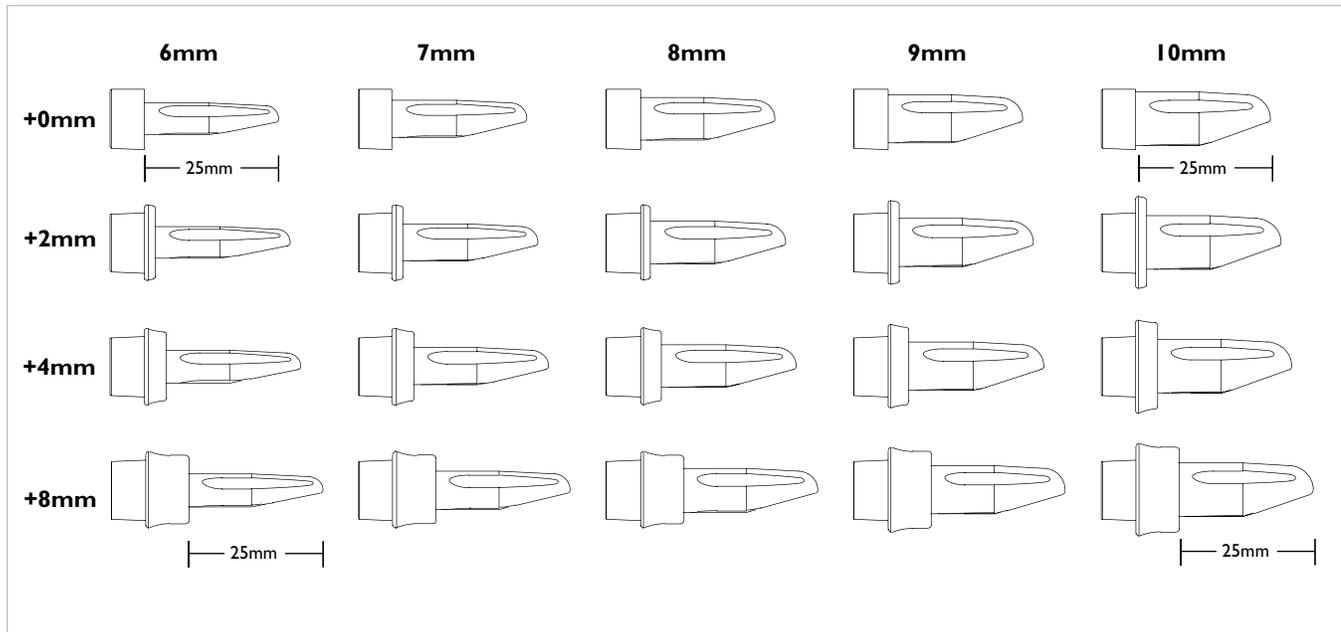

***Optional +6mm stems and trials are available upon request.**



The innovative broaches in the Anatomic Radial Head System allow the surgeon to create a precise opening in the radial canal for proper insertion of the implant. The broaches enter the radial canal in a straight direction and are less likely to broach the canal at an angle, resulting in improper implant placement. Spiral flutes on the broach are designed to displace bone during broaching. The implant stem is 0.5mm oversized from the broach diameter. The trial stem diameter is 0.5mm undersized of the broach diameter to allow for ease of trial insertion and removal.


A mallet should be used to insert the broach. Side Pegs are provided for removal with a mallet and also provide a T-Handle to ease broach insertion and extraction. Furthermore, the broaches are color-coded for ease of trial implant selection. Collar reamers are included in the system to create a perpendicular neck surface for the stem facilitating accurate placement of the stem.



A unique guide allows the surgeon to determine proper collar height. A sizing gauge is placed in the radial canal and then ratcheted proximally with the collar sizing gauge. The measurement corresponds to proper collar height for accurate restoration of radial length.



Anatomic Radial Head

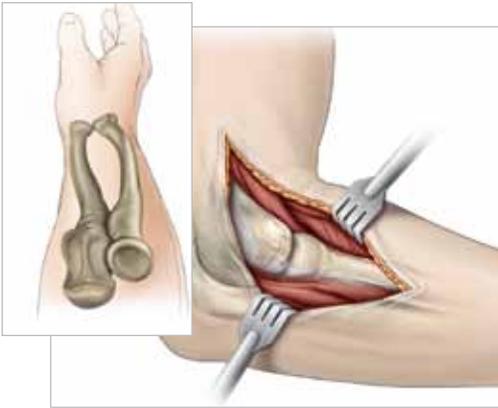

1 Incision and Dissection:

While there are many acceptable exposure methods, the Kaplan interval in a line from the lateral epicondyle toward Lister's tubercle, with the forearm in neutral rotation, permits the collateral ligament to be left intact. In fracture dislocations, the exposure is through the traumatic opening in the ligament complex. Proximally, the ECRL origin is released with the anterior capsule to permit direct access to the front of the radial head.



2 Radial Head Resection:

Template the radial head prior to surgery to determine the appropriate level of resection. Resect the radial head with a microsagittal saw as close to the surgical neck as possible. A maximum length of 17mm of the radius can be replaced. This 17mm includes the radius length reamed with the Collar Reamer in Step 4.



3 Determine Stem Diameter:

Use the 5mm awl (TR-0206) to initially enter the canal. Starting with the smallest broach (6mm, TR-BRA06), prepare the canal for the stem. Use sequentially larger broaches until a tight fit is achieved with the broach. Tap on the back end of the broach with a mallet. There is a groove on the broach just above the cutting flutes that indicates when to stop. Note that the broaches are 0.5mm undersized from the implant stem to ensure a tight press fit.



4 Ream with Collar Reamer:

Select the collar reamer (TR-CRAxx) that matches the stem diameter determined by the broach in the previous step. Under power or by hand, ream to create a surface where at least 60% of the radial shaft is in contact with the reamer. To ream by hand, attach the collar reamer to the T-Handle (MS-T1212). Do not over-ream the radial shaft; removing too much bone will cause the radial head not to articulate properly with the capitellum.

5 Determine Head Diameter:

Determine head diameter by placing the resected head into the sizing pockets on the impactor base (TR-MS03). If between sizes, select the smaller diameter.



6 Assemble Head and Stem Gauge:

Assemble the head gauge (TR-TG02) and stem gauge (TR-TGA06). The head gauge needs to be completely compressed.



7 Determine Collar Height:

Insert stem gauge assembly (TR-TGA06) into the bone canal. Starting with the +0 end of the trial gauge (TR-TG01), sequentially increase the height by inserting the end of the gauge under the head of the assembly, until the head reaches the capitellum. It is critical that the coronoid contacts the trochlea during this process. The coronoid separated from the trochlea is an indicator that the collar is too large. The number on the trial gauge (+0, 2, 4, 8mm) will correspond to the collar height on the stem.



8 Select Trial Implants and Assemble:

After selecting the trial head and stem, align laser marks on the head and stem and assemble using hand pressure. The stem laser mark is indicated for Left and Right for proper orientation. If the trial head and stem are difficult to connect, apply saline solution prior to connecting.





9 Trial Implant Insertion:
Insert the trial implant into the radius. Ensure that the laser marks on the head and stem are aligned with the lateral aspect of the radius when the forearm is in neutral position. Lister's tubercle may also be used as a landmark for laser mark orientation. Check for proper articulation with the capitellum and the coronoid. The coronoid needs to be in contact with the trochlea to ensure proper positioning of the trial. The trial stems are 0.5mm undersized from the broaches for ease of insertion.



10 Implant Assembly:
After determining the correct size head and stem with the trials, place the implant stem into the appropriate size hole in the impactor base (TR-MS03). Align laser marks and impact the head and stem, then lock the Morse taper using the impactor (TR-MS05) and a mallet.



11 Implant Insertion:
Insert the implant into the radius using the impactor (TR-MS05) and a mallet. Ensure that the laser mark on the head is aligned with the lateral aspect of the radius when the forearm is in neutral position. Lister's tubercle may also be used as a landmark for laser mark orientation. A stem removal tool (TR-MS30) is available in the system if needed.



12 Postoperative Protocol:
Postoperative management is determined by the overall management of the elbow and limb, more so than specifically the radial head. For isolated fractures of the radial head and neck, without ligament injury, early motion is commenced in flexion and extension as well as pronation and supination. This usually begins within the first few days after surgery.

Heads

20.0mm Head, Right	TR-H200R-S
22.0mm Head, Right	TR-H220R-S
24.0mm Head, Right	TR-H240R-S
26.0mm Head, Right	TR-H260R-S
28.0mm Head, Right	TR-H280R-S
20.0mm Head, Left	TR-H200L-S
22.0mm Head, Left	TR-H220L-S
24.0mm Head, Left	TR-H240L-S
26.0mm Head, Left	TR-H260L-S
28.0mm Head, Left	TR-H280L-S

Stems

6.0mm x 0.0mm Stem	TR-S0600-S
6.0mm x 2.0mm Stem	TR-S0602-S
6.0mm x 4.0mm Stem	TR-S0604-S
6.0mm x 8.0mm Stem	TR-S0608-S
7.0mm x 0.0mm Stem	TR-S0700-S
7.0mm x 2.0mm Stem	TR-S0702-S
7.0mm x 4.0mm Stem	TR-S0704-S
7.0mm x 8.0mm Stem	TR-S0708-S
8.0mm x 0.0mm Stem	TR-S0800-S
8.0mm x 2.0mm Stem	TR-S0802-S
8.0mm x 4.0mm Stem	TR-S0804-S
8.0mm x 8.0mm Stem	TR-S0808-S
9.0mm x 0.0mm Stem	TR-S0900-S
9.0mm x 2.0mm Stem	TR-S0902-S
9.0mm x 4.0mm Stem	TR-S0904-S
9.0mm x 8.0mm Stem	TR-S0908-S
10.0mm x 0.0mm Stem	TR-S1000-S
10.0mm x 2.0mm Stem	TR-S1002-S
10.0mm x 4.0mm Stem	TR-S1004-S
10.0mm x 8.0mm Stem	TR-S1008-S

Instruments

6mm Broach Assembly	TR-BRA06
7mm Broach Assembly	TR-BRA07
8mm Broach Assembly	TR-BRA08
9mm Broach Assembly	TR-BRA09
10mm Broach Assembly	TR-BRA10
Trial Gauge	TR-TG01
Head Gauge	TR-TG02
6.0mm Stem Gage Assembly	TR-TGA06
20mm Trial Head, Left	TR-TH20L
20mm Trial Head, Right	TR-TH20R
22mm Trial Head, Left	TR-TH22L
22mm Trial Head, Right	TR-TH22R
26mm Trial Head, Left	TR-TH26L
26mm Trial Head, Right	TR-TH26R
28mm Trial Head, Left	TR-TH28L
28mm Trial Head, Right	TR-TH28R
6.0mm x 0.0mm Trial Stem	TR-TS60
6.0mm x 2.0mm Trial Stem	TR-TS62
6.0mm x 4.0mm Trial Stem	TR-TS64
6.0mm x 8.0mm Trial Stem	TR-TS68
7.0mm x 0.0mm Trial Stem	TR-TS70
7.0mm x 2.0mm Trial Stem	TR-TS72
7.0mm x 4.0mm Trial Stem	TR-TS74
7.0mm x 8.0mm Trial Stem	TR-TS78
8.0mm x 0.0mm Trial Stem	TR-TS80
8.0mm x 2.0mm Trial Stem	TR-TS82
8.0mm x 4.0mm Trial Stem	TR-TS84
8.0mm x 8.0mm Trial Stem	TR-TS88
9.0mm x 0.0mm Trial Stem	TR-TS90
9.0mm x 2.0mm Trial Stem	TR-TS92
9.0mm x 4.0mm Trial Stem	TR-TS94
9.0mm x 8.0mm Trial Stem	TR-TS98
10.0mm x 0.0mm Trial Stem	TR-TS100
10.0mm x 2.0mm Trial Stem	TR-TS102
10.0mm x 4.0mm Trial Stem	TR-TS104

Ordering Information

Instruments

10.0mm x 8.0mm Trial Stem	TR-TS108
Head Impactor	TR-MS05
Impactor Base	TR-MS03
6mm Collar Reamer	TR-CRA06
7mm Collar Reamer	TR-CRA07
8mm Collar Reamer	TR-CRA08
9mm Collar Reamer	TR-CRA09
10mm Collar Reamer	TR-CRA10
Quick Release T-Handle	MS-T1212
5.5mm Quick Release Awl	TR-0206
Stem Removal Tool	TR-MS30
Total Radial System Tray	TR-0001

Optional Items

6.0mm x 6.0mm Stem	TR-S0606-S
7.0mm x 6.0mm Stem	TR-S0706-S
8.0mm x 6.0mm Stem	TR-S0806-S
9.0mm x 6.0mm Stem	TR-S0906-S
10.0mm x 6.0mm Stem	TR-S1006-S
6.0mm x 6.0mm Trial Stem	TR-TS66
7.0mm x 6.0mm Trial Stem	TR-TS76
8.0mm x 6.0mm Trial Stem	TR-TS86
9.0mm x 6.0mm Trial Stem	TR-TS96
10.0mm x 6.0mm Trial Stem	TR-TS106
TRH 6mm Collar Trial Tray Insert	80-0181



Acutrak 2® Mini & Micro Instruments

Acutrak 2® Tray Mini Screw Module	AT2-006
AT2 Micro Instrument Module	80-0405
Mini-Acutrak 2® Drill	AT2M-1813
Mini-Acutrak 2® Drill, Long	AT2M-L1813
Micro-Acutrak 2® Drill	AT2-1509
Micro-Acutrak 2 Drill, Long	80-0100
2.0mm Cannulated Quick Release Driver Tip	HT-1120
1.5mm Cannulated Quick Release Driver Tip	HT-0915
.045" x 6" ST Guide Wire	WS-1106ST
.035" x 5.75" ST Guide Wire	WS-0906ST
.045 Diameter, Parallel Wire Guide Assembly	AT2-4500
.035 Diameter, Parallel Wire Guide Assembly	AT2-3500

The Anatomic Radial Head System may also be used in combination with the following Acumed® Products:

- Locking Radial Head Plate System
- Acutrak 2® Headless Compression Screw System (Mini & Micro)

For ordering information, please contact your local Acumed® Sales Representative.

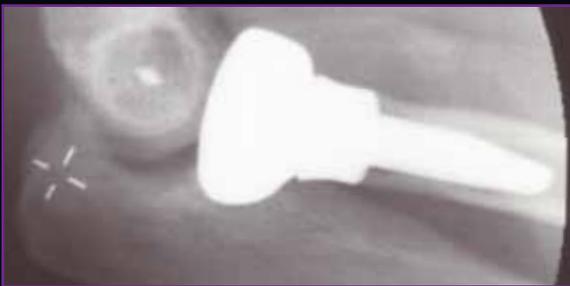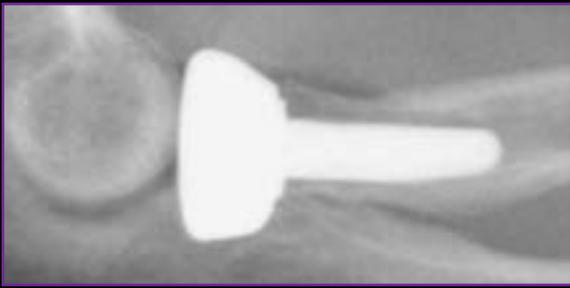

1: van Riet RP, van Glabbeek F, Baumfeld A, Neale PG, Morrey BF, O'Driscoll SW, An KN. The effect of the orientation of the radial head on the kinematics of the ulnohumeral joint and force transmission through the radio capitellar joint. *Clin Biomech* (Bristol, Avon). 2006 Mar 9

2: van Riet RP, van Glabbeek F, Baumfeld A, Neale PG, Morrey BF, O'Driscoll SW, An KN. The effect of the orientation of the noncircular radial head on elbow kinematics. *Clin Biomech* (Bristol, Avon). 2004 Jul;19(6):595-9.

3: van Riet RP, van Glabbeek F, Neale PG, Bimmel R, Bortier H, Morrey BF, O'Driscoll SW, An KN. Anatomical considerations of the radius. *Clin Anat*. 2004 Oct;17(7):564-9.

4: van Riet RP, van Glabbeek F, Neale PG, Bortier H, An KN, O'Driscoll SW. The noncircular shape of the radial head. *Hand Surg*. 2003 Nov;28(6):972-8.

5: Swieszkowski W, Skalski K, Pomianowski S, Kedzior K. The anatomic features of the radial head and their implication for prosthesis design. *Clin Biomech* (Bristol, Avon). 2001 Dec;16(10):880-7

6: King G, Zarzour ZD, Patterson SD, Johnson A. An anthropometric study of the radial head: implications in the design of a prosthesis. *Arthroplasty*. 2001 Jun;16(1):112-6.

7: van Glabbeek F, van Riet RP, Baumfeld A, Neale PG, O'Driscoll SW, Morrey BF, An KN. Detrimental effects of overstuffing or understuffing with a radial head replacement in the medial collateral-ligament deficient elbow. *Bone Joint Surg Am*. 2004 Dec;86-A(12):2629-35.

8: van Glabbeek F, van Riet RP, Baumfeld A, Neale PG, O'Driscoll SW, Morrey BF, An KN. The kinematic importance of radial neck length in radial head replacement. *Med Eng Phys*. 2005 May;27(4):336-42.

9: Moro A, Werier M, MacDermid A, Patterson SD, King G. Arthroplasty with a metal radial head for unreconstructible fractures of the radial head. *Bone Joint Surg Am*. 2001 Aug;83-A(8):1201-11.

10: Popovic N, Djekic M, Lemaire R, Gillet P. A comparative study between proximal radial morphology and the floating radial head prosthesis. *Shoulder Elbow Surg*. 2005 Jul-Aug;14(4):433-40.

11: Data on file

ACUMED[®]

5885 NW Cornelius Pass Road
Hillsboro, OR 97124
(888) 627-9957
www.acumed.net

Distributed by:

These materials contain information about products that may or may not be available in any particular country or may be available under different trademarks in different countries. The products may be approved or cleared by governmental regulatory organizations for sale or use with different indications or restrictions in different countries. Products may not be approved for use in all countries. Nothing contained on these materials should be construed as a promotion or solicitation for any product or for the use of any product in a particular way which is not authorized under the laws and regulations of the country where the reader is located. Specific questions physicians may have about the availability and use of the products described on these materials should be directed to their particular local sales representative. Specific questions patients may have about the use of the products described in these materials or the appropriateness for their own conditions should be directed to their own physician.

Effective 07/2010

ELB00-04-A